Quanterix
The Science of Precision Health

Simoa® PD-L1 Discovery Kit
Certificate of Analysis

Product Number:	102648
Lot Number:	503525
Expiration:	23-May-2023
Platform(s):	HD-1/HD-X & SR-X

Data below represents results generated on the Simoa® HD-X Analyzer.

Component	Part Number	Lot Number
Bead Stock	102641	219402
Detector Stock	102642	219503
Calibrator Concentrate	102645	223711
Calibrator Diluent	102643	218616
Sample Diluent	102644	219408
Detector Diluent	102734	219502

Generic Components - Included With Kit But Not Lot Number Specific	
Discovery Bead Diluent	101954
Discovery SBG Diluent	101956
Discovery SBG Stock	103297
RGP Reagent	103159

Calibrator Concentrate Target Value (pg/mL)	3000

Calibration Curve

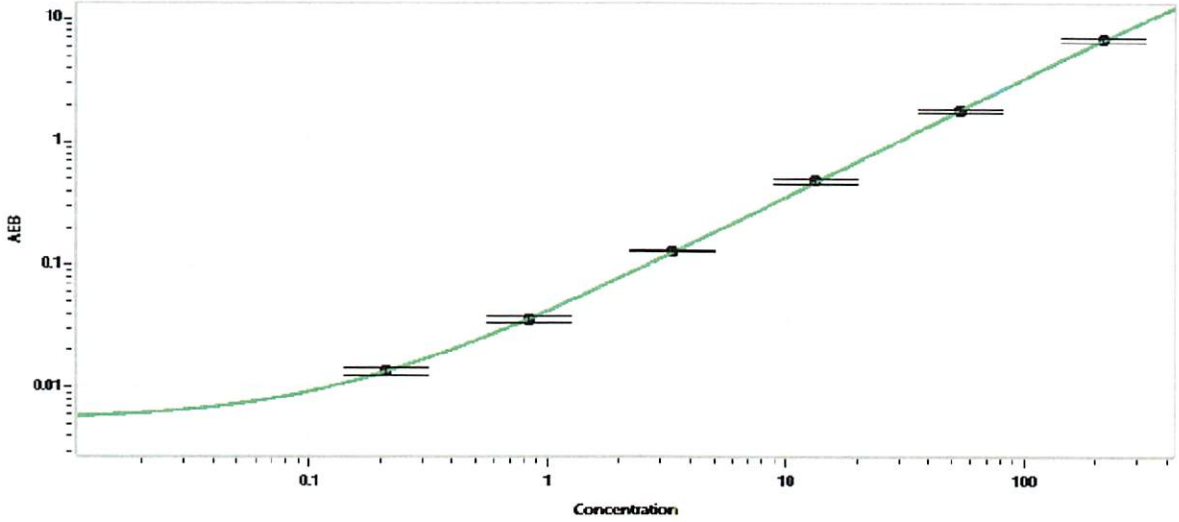

Calibrator Levels (pg/mL)	
A	0.000
B	0.210
C	0.840
D	3.36
E	13.4
F	53.8
G	215

Review/Approval

Name	Title	Signature/Date
Sonia Khillan	QC Manager	Sonia Khillan / 13SEP2022

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnositic procedures