Quanterix
The Science of Precision Health

Simoa® HIV p24 Kit
Certificate of Analysis

Product Number:	102215
Lot Number:	503550
Expiration:	3-Aug-2023
Platform(s):	HD-1/HD-x & SR-X

Component	Part Number	Lot Number
Bead Reagent	102211	222708
Detector Reagent	102212	223507
SBG Reagent	102213	222806
Assay Diluent	102214	222807
Calibrators	101310	224201
Control 1	100702	224202
Control 2	100703	224202
RGP Reagent	103159	N/A[1]

[1] RGP is not Kit Lot Specific

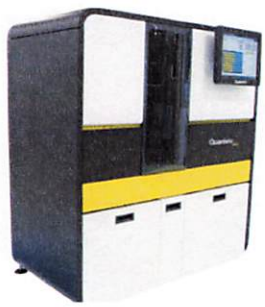

Data below represents results generated on the Simoa® HD-X Analyzer.

Release Materials*			
	Lot	Result (pg/mL)	Spec. Range (pg/mL)
Control 1	224202	0.100	0.084 - 0.126
Control 2	224202	12.9	9.23 - 13.8
Panel 1	019601	0.220	0.127 - 0.243
Panel 2	019601	2.21	1.56 - 2.34
Panel 3	019601	13.7	9.44 - 14.2

* Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.

Calibration Curve

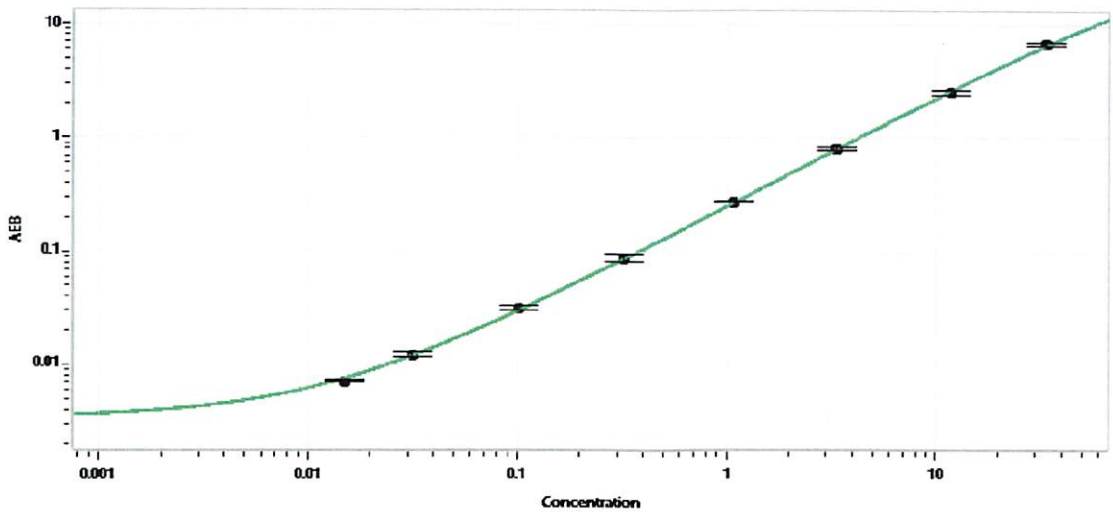

Calibrator Levels (pg/mL)	
A	0.000
B	0.015
C	0.032
D	0.102
E	0.322
F	1.08
G	3.37
H	11.8
I	33.6

Review/Approval Sonia Khillar — QC — 12/11/- /08 NOV 2022

Name — Title — Signature/Date

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnositic procedures