Quanterix
The Science of Precision Health

Simoa® GFAP Discovery Kit
Certificate of Analysis

Product Number:	102336
Lot Number:	503767
Expiration:	14-Dec-2023
Platform(s):	HD-1 / HD-X & SR-X

Data below represents results generated on the Simoa® HD-1 / HD-X& SR-X Analyzer.

Component	Part Number	Lot Number
Bead Stock	102330	300601
Detector Stock	102331	300901
Calibrator Concentrate	102335	302604
Calibrator Diluent	102332	234815
Sample Diluent	102333	300902

Generic Components - Included With Kit But Not Lot Number Specific		
Discovery Bead Diluent	101954	N/A
Discovery Detector Diluent	101955	N/A
Discovery SBG Diluent	101956	N/A
Discovery SBG Concentrate	103297	N/A
RGP Reagent	103159	N/A

Calibrator Concentrate Target Value (ng/mL)	20 ng/mL

Calibration Curve

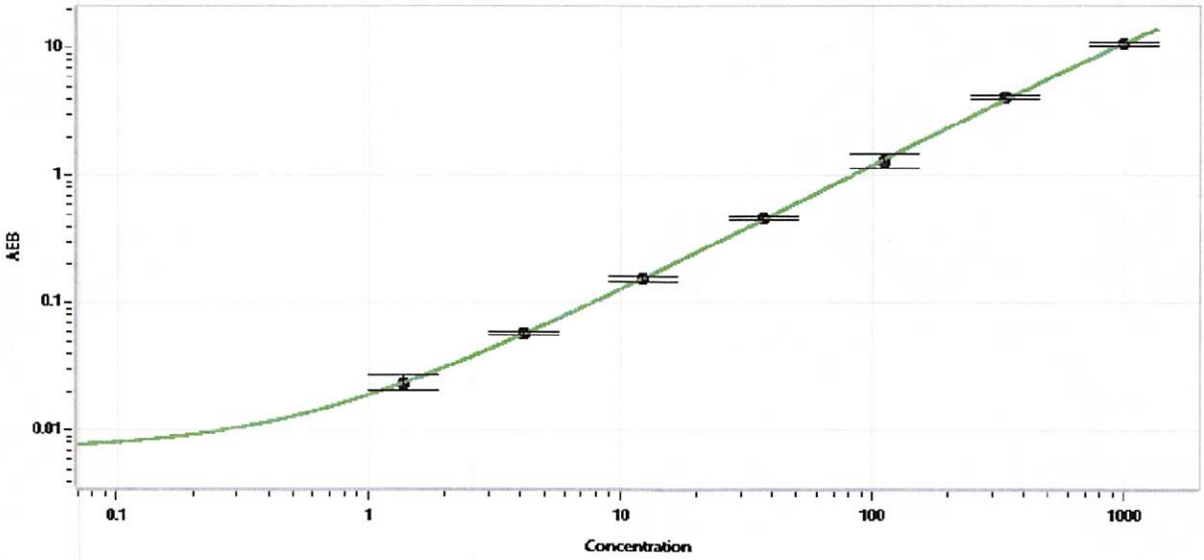

Calibrator Levels (pg/mL)	
A	0.000
B	1.37
C	4.11
D	12.3
E	37.0
F	111
G	333
H	1000

Review/Approval

Name	Title	Signature/Date
Sonia Khillan	QC Manager	Sonia Khillan 22 MAR 2023

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, MA 01821
techsupport@quanterix.com

©Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures