Quanterix®

Discovery Fueled by Ultra-Sensitivity

Simoa® IL-10 2.0 Kit

Certificate of Analysis

Product Number:	101643
Lot Number:	504284
Expiration:	16-Jan-2025
Platform(s):	SR-X and HD-1/HD-X

Data below represents results generated on the

Component	Part Number	Lot Number	Control Lot Number
Bead Reagent	101645	415501	N/A
Detector Reagent	101644	415502	N/A
SBG Reagent	101646	423906	N/A
Sample Diluent	102200	401621	N/A
Calibrator Diluent	101648	415505	N/A
Calibrator Concentrate	100670	315305	315305A
SBG Diluent (SR-X)†	103158	N/A[1]	N/A[1]
RGP Reagent	103159	N/A[1]	N/A[1]

[1] Reagents are not Kit Lot Specific

† Specific to use on the SR-X platform.
Refer to the IL-10 Kit Instructions - SR-X (KI-0036).

Release Materials*			
	Lot	**Result (pg/mL)**	**Spec. Range (pg/mL)**
Control 1	315305A	23.4	18.0 - 30.0
Control 2	315305A	1.49	1.20 - 2.00

*** Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.**

Calibrator Concentrate Value Assignment (pg/mL)	603

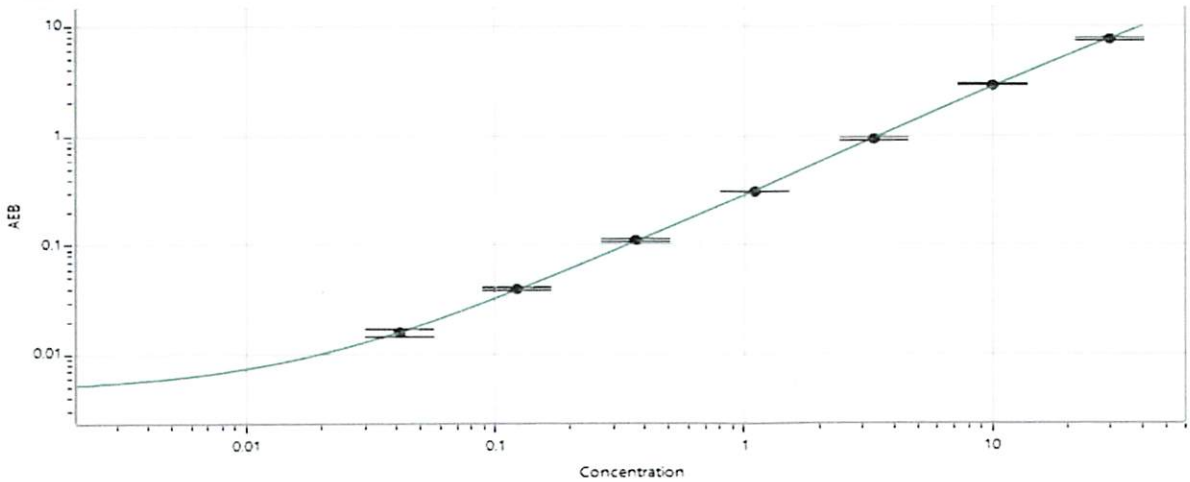

Calibrator Levels (pg/mL)	
A	0.000
B	0.041
C	0.123
D	0.370
E	1.11
F	3.33
G	10.0
H	30.0

Review/Approval Dilesh Patel — Doc control-II QA — [signature] / 13SEP2024

Name **Title** **Signature/Date**

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, 01821
techsupport@quanterix.com

©2024 Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures.