Quanterix®

Discovery Fueled by Ultra-Sensitivity

Simoa® NF-Light v2 Advantage Kit

Certificate of Analysis

Product Number:	104073
Lot Number:	504471
Expiration Date:	26-May-26
Platform(s):	SR-X and HD-1/HD-X

Component	Part Number	Lot Number
Bead Reagent	104067	433103
Detector Reagent	104068	433201
SBG Reagent	104069	434702
Sample Diluent Reagent	104071	433712
Reference Calibrators	102255	434401
Control 1	102256	434402
Control 2	102257	434402
RGP Reagent	103159	N/A[1]

[1] Reagents are not Kit Lot Specific

Data below represents results generated on the Simoa® HD-X Analyzer.

Release Materials*

NF-Light®

	Lot	Result (pg/mL)	Spec. Range (pg/mL)
Control 1	434402	4.43	3.20 - 4.91
Control 2	434402	299	252 - 377

*** Ranges shown are generated internally for new lot release only. Customer should generate their own control ranges.**

Calibration Curve

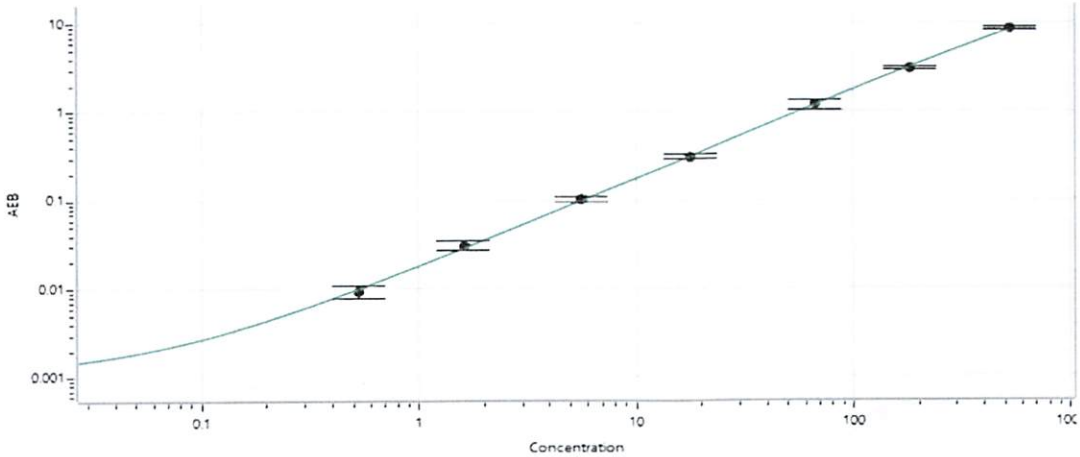

Calibrator Levels (pg/mL)	
A	0.000
B	0.531
C	1.61
D	5.57
E	17.7
F	66.8
G	182
H	526

Review/Approval Dilesh Patel — Doc control II-QA — 06Feb2025

Name — Title — Signature/Date

Quanterix Corporation
900 Middlesex Turnpike, Building 1, Billerica, 01821
techsupport@quanterix.com

©2025 Quanterix Corp. Simoa® is a registered trademark of Quanterix Corp.
For research use only. Not for use in diagnostic procedures.

COA-0049 02